

## PARALELAS STANDARD - F.51-S

Graduables en altura y anchura hasta quedar plegada.

La altura de las bases del suelo se ha reducido al máximo, facilitando el paso a la zona de marcha.

Estructura metálica, rematada en cromo y poliéster.

Longitud 300 cm.

## STANDARD PARALLEL BARS – F.51-S

Adjustable height and width (until totally folded).

The height of the base off the floor has been reduced to a minimum to allow for easy access to the walkway.

Metal frame with chrome and epoxy finish.

Length: 300 cm.



### INSTRUCCIONES DE MONTAJE / ASSEMBLY MANUAL




Última revisión 17/10/2014

## RECOMENDACIONES DE USO / RECOMMENDATIONS FOR USE

Debe instalarse paralelamente a una de las paredes del gimnasio pero a suficiente distancia como para que el fisioterapeuta pueda moverse mientras camina con el paciente. Se colocará un espejo en la pared en uno o ambos extremos de modo que el enfermo pueda verse y coordinarse deambulando. Pasada esta fase de deambulación podremos continuar con rampa y escalera. Siga cuidadosamente todas las instrucciones dadas por su médico, fisio o terapeuta para el uso del producto.

*Must be installed in parallel to the walls of the gym but at enough distance so that the physiotherapist can move while the patient is walking. It will be place a mirror on the wall in one or both ends so that the patient might see himself and coordinated wandering. Passed this stage of wandering we can continue with ramp and stairs. Follow carefully all instructions given by your doctor, physic or therapist for the use of the product.*

## INSTRUCCIONES DE MONTAJE / ASSEMBLY INSTRUCTIONS

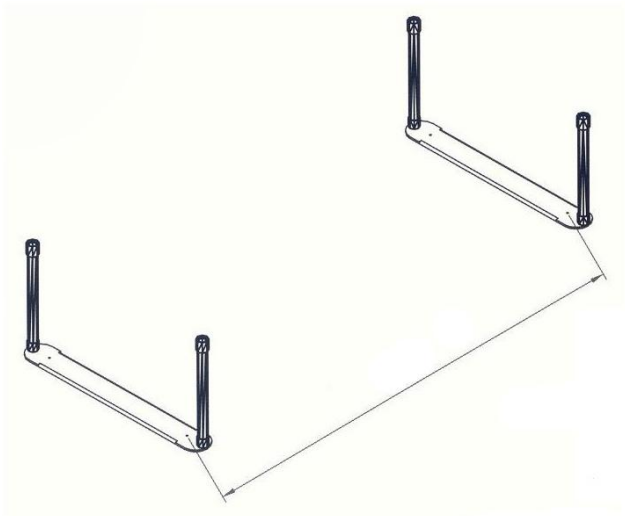

1. Las paralelas se suministran con los tubos tinteros en las bases lastradas. Colocar las bases lastradas a la distancia indicada en la sección de medidas de cada paralela.

*1 The parallels are supplied with hollow tubes in the weighted basis. Place the weighted basis at the distance indicated in the measure section of each parallel.*




2 Situar los pasamanos dentro de los tubos tinteros y seleccionar la altura deseada introduciendo las clavijas en los agujeros correspondientes. (Ver detalle).

*2 Place the handrails inside the hollow tubes and select the desired height inserting the plugs in the appropriate holes (see detail)*



NOTA. Para plegar las paralelas el plano separador, luego plegar en el sentido de las flechas según se muestra, llevando el pasamanos A hacia el pasamanos B.

*NOTE. To fold the parallels remove the abduction board, then do it in the direction of the arrows as shown, bringing the handrail A into the handrail B.*

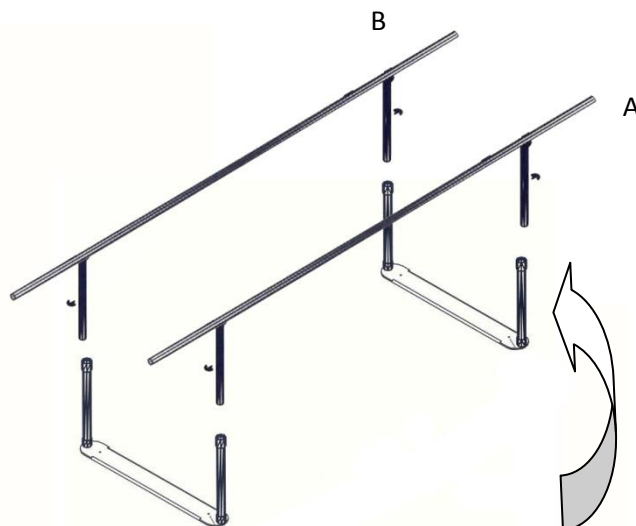

APARATOS Y DISPOSITIVOS  
PARA APLICACIONES TERAPEUTICAS

**ORTOTECSA**

ORTOTECSA, S.L.

C/.Peña de Francia,8 (28500) Arganda del Rey  
MADRID (España)

Tlf: +34 918 719 132 / Fax: +34 918 719 323

E-mail: [info@ortotecsa.com](mailto:info@ortotecsa.com)

Web: [www.ortotecsa.com](http://www.ortotecsa.com)